

***Sarve Bhavantu Sukhina***  
***Sarve Santu Niramaya***

# ABOUT US

**Aurus MedTech** derives its name from the Latin word "Aurum" that means GOLD. Just as gold has been a sign of purity and high quality since the early days of civilisation. We at Aurus have embibed the same values in our Products and Processes. We aim to be the Gold Standard in Medical Devices in the coming years.



Driven by innovation and a Strong sense of service we pride for the care and precision with which we make each and every product. A team of engineers that is constantly developing new products, we are dedicated and committed to the service of humanity.

In an ever changing Healthcare ecosystem, we constantly strive to be at the fore-front of patient care. When it comes to Patient care, quality is of the almost importance. Keeping this mind, we at Aurus, have an experienced team of engineers dedicated to Quality Assurance & Quality Control.

A manufacturing plant that boasts of state of the art Equipment within a 4500 sq. ft. ISO Class 7 Clean Room, we use cutting edge technology for manufacturing of our Medical Devices, ensuring the highest standards and productivity. Our plant and the manufacturing process is EN ISO 13485:2016 Certified and our Products are CE Certified. Ensuring the best quality and following WHO:GMP compliance.

Our Products portfolio enables clinicians to be more efficient and effective in treating patients at the hospital bedside, in the operating theater, in critical care units, at home and in the dialysis clinic. We are working alongside our partners to find new and smarter ways to improve patient outcomes, prevent complications before they become life-threatening and increase access to care, while reducing total costs.





***Sarve Bhavantu Sukhina***  
***Sarve Santu Niramaya***

About Company

Our Mission

Research & Development





 INFUSION THERAPY	2,3,4,5
 CARDIOVASCULAR	6,7
 CRITICAL CARE	8
 NEPHROLOGY	9
 SURGERY AND DRAINAGE	10
 UROLOGY	11
 GASTROENTEROLOGY	12
 ANAESTHESIA & RESPIRATORY CARE	13
 CERTIFICATED	14



**AURUS DEVICES**

# INFUSION THERAPY

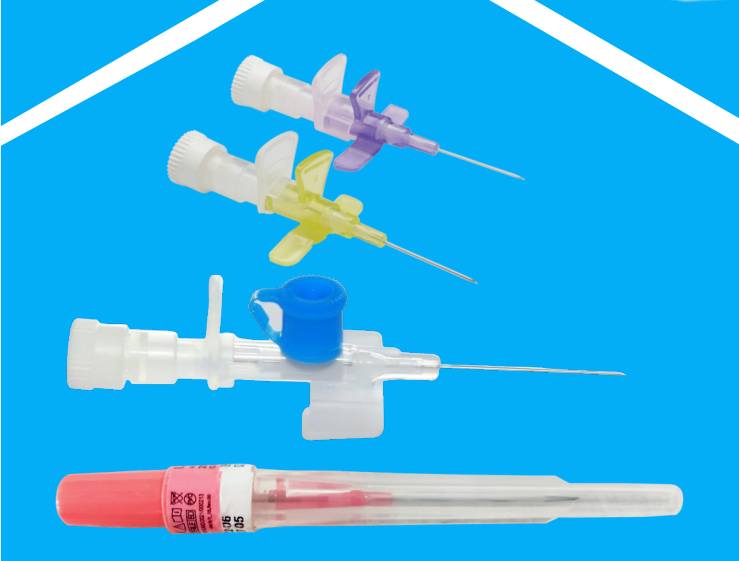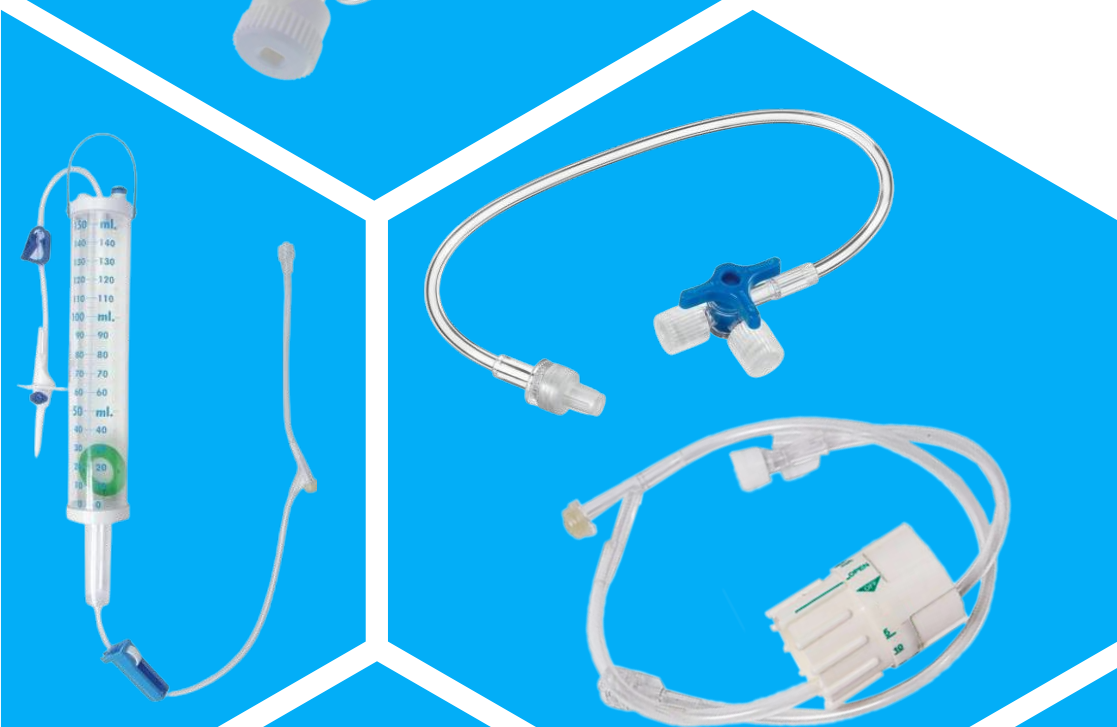

# INFUSION THERAPY

## RANGE OF IV CANNULA

### AURFLON

- Instant flash back and minimizes blood exposure.
- Available in PTFE & FEP.
- 6% luer taper for compatibility with all standard devices.
- With Tri-Sectional Bevel Needles.
- Rounded Grip needle hub for better support.
- Stainless Steel, Silicone Tipped needle for smooth penetration.
- Port cap is color coded as per ISO 10555-Part5.



ITEM CODE:IT0101E\*



Additional Port Cap  
For Medication



Tricut Bevel Needle



6% Taper Luer  
Lock Connection



Smooth Wings For  
Easy Fixation



ITEM CODE:IT0102E\*

### AURNEO

- Design for Paediatric Cannula.
- Design without any Injection Port.
- Mini-Wings for secure fixation.
- A small Projection on main body for easy handling of cannula.
- Available only in 24 & 26G.
- Wing is color coded as per ISO 10555-Part5.

### AURPEN

- Catheter tip is designed for a smooth Cannulation.
- Transparent / Clear Flash Back chamber confirms quick flashback.
- Designed with broad needle hub for perfect grip and control over the catheter.
- Universal 6% taper for compatibility with any other standard medical device.
- Radiopaque Stripes helps to detect under X-Ray.



ITEM CODE:IT0103E\*

## GAUGE OF COLOUR CODE



14G  
Orange



16G  
Medium gray



17G  
White



18G  
Dark Green



20G  
Pink



22G  
Deep Blue



24G  
Yellow



26G  
Purple



ITEM CODE:IT0201A\*

## RANGE OF INFUSION SETS DRIPCARE-IV

- ⦿ Round collapsible drip chamber to facilitate fluid level adjustment and drop count.
- ⦿ Disc type fluid filter provide in drip chamber for fluid filtration for any particulate matters.
- ⦿ Strong & Sharp Spike for easy insertion in to IV container.
- ⦿ Kink resistant PVC tubing facilitate with efficient thumb roller clamp for accurate and unrestricted flow.
- ⦿ Drop rate -20 drop/ml.



ITEM CODE:IT0203A\*

## DRIPCARE-V


- ⦿ Hydrophobic filter to prevent entry of air born micro organism.
- ⦿ Big roller clamp for accurate and unrestricted flow.
- ⦿ Self-sealing latex bulb for extra medication.
- ⦿ Big Drip Chamber with air vent.
- ⦿ Kink resistant PVC tubing
- ⦿ Packed in Ribbon Pouch.



ITEM CODE:IT0204A\*

## DRIPCARE +

- ⦿ IV infusion set with Airvent, 150cm kink-resistant tube, connected with Y injection site, with luer lock
- ⦿ Same as Dripcare V
- ⦿ Packed in Ribbon Pouch.

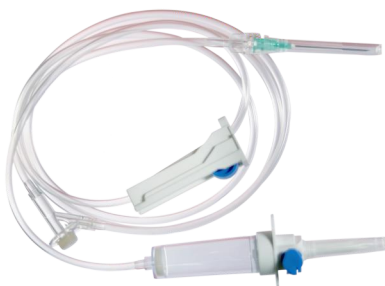

ITEM CODE:IT0207A\*

## DRIPCARE - UNIQUE

- ⦿ IV infusion set with Airvent, 150cm kink-resistant tube, connected with Y injection site, with Rotating Combi-lock.
- ⦿ DEHP Free Tubing.
- ⦿ Packed in Ribbon Pouch.



ITEM CODE:IT06E\*

### 3 WAY STOP COCK

- ⦿ Available in standard and Lipid Resistant Variant, the 360 degree rotating stopcock is with transparent channel.
- ⦿ Minimum priming volume required for accurate drug administration.
- ⦿ Rotating male luer and two female luer connectors.
- ⦿ Arrow on the handle to indicate the direction of flow.
- ⦿ Leakage free fitment for pressure up to 4.5 bar (65psi).
- ⦿ **Available in Blue, Red & White colours**

### 3 WAY STOPCOCK WITH EXTENSION LINESS



ITEM CODE:IT07C\*

- ⦿ Soft PVC kink resistant tubes available in 10, 15, 20, 25, 50, 75, 100, 150, 200cms.
- ⦿ Tube ID-3mm and OD-4mm.
- ⦿ Connected with rotating luer lock.
- ⦿ Also available in microbore with 2mm ID.



ITEM CODE:IT09C\*

### EXTENSION LINES / PM LINE

- ⦿ Extension tube provides separation of administration and insertion sites.
- ⦿ Available in various tube lengths on customer requirements.
- ⦿ Available in Male-Female, Female - Female and Male - Male port . Variant:- Length 10, 20, 50, 100, 150 & 200cm.



ITEM CODE:IT03C\*

### I.V. FLOW REGULATOR

- ⦿ Designed to control the rate of intravenous fluid manually. It ensures the accurate replacement of I.V. fluid from infusion to patients I.V. Cannula.
- ⦿ Precies control of flow rate of IV fluids with a range of 0 to 250 ml/hr, With "Y" injection port for intermittent medication.
- ⦿ Soft and kink resistant PVC tubing.
- ⦿ Standard tube length: without "Y" site: 20cm & with "Y" site: 40cm. Tube dia. IØ3.0mm, OØ4.1mm.
- ⦿ Available with infusion set also.



ITEM CODE:IT08B\*

## PAEDIA VOL

(Paedia Drip Measured Volume Set)


- ⦿ Cylinder, flexible, clear and calibrated measured volume chamber in size 110/150ML.
- ⦿ Unique floating auto shut off valve act as a floating indicator and automatically shuts off the drain path to prevent the passage of air in the line.
- ⦿ Soft and kink resistance PVC tube, 150 cm long.



ITEM CODE:CC02E\*

## NEEDLE FREE CONNECTORS

- ⦿ Solo-Line - Swabable Needle free site made up of Silicon with almost dead space. Prevents microbial invasions & Made in compliance with 6% Luer taper.
- ⦿ Uni-Line - one needle free site with extension line. and with combi-lock & Slide clamp. I.D. 1.2mm & O.D. 2.5mm
- ⦿ Bi-Line - two needle free site with extension line and combi-lock & Slide clamp. Non DEHP tube. I.D. 1.2mm & O.D. 2.5mm.
- ⦿ Tri-Line - With extension line and three needle free injection site. I.D. 1.2mm & O.D. 2.5mm. With combi-lock & Slide clamp. Non DEHP tube.

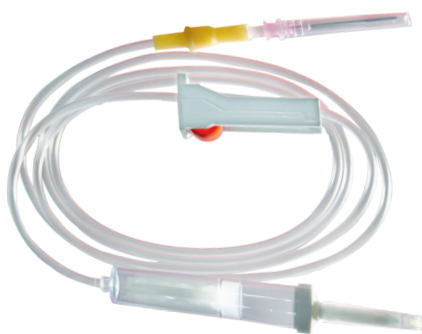


ITEM CODE:NL01B\*

## BLOOD TRANSFUSION SET

- ⦿ For transfusion of blood or blood components.
- ⦿ Soft, flexible and transparent drip chamber.
- ⦿ soft and kink resistant DEHP free PVC Tube.
- ⦿ Latex bulb for intermittent medication.
- ⦿ Effective roller controller for precise adjustment of the flow rate.
- ⦿ 18G Hypodermic Needle




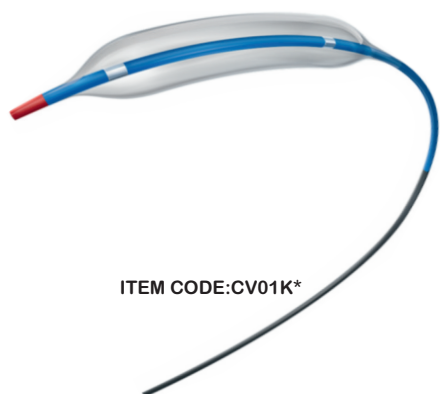

ITEM CODE:CV01K\*

## PTCA BALLOON DILATATION CATHETER

- ⊙ TACHY CTO (RX type), a Semi-Compliant pre-dilatation balloon catheter with diameter sizes of 1.0mm-4.0mm, is designed for CTO and other chronic coronary stenosis.
- ⊙ It is featured of extraordinary crossability, flexibility, pushability and rewrap.

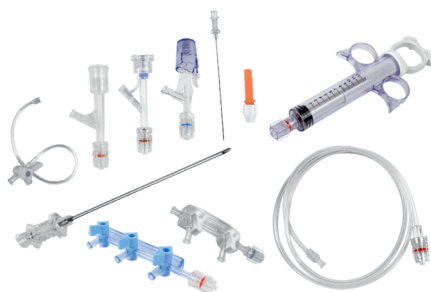

ITEM CODE:CV02C\*

## PTCA KIT


- ⊙ PTCA Kit is used in Angioplasty.
- ⊙ Percutaneous transluminal coronary angioplasty (PTCA) is a minimally invasive procedure to open up blocked coronary arteries, allowing blood to circulate without any obstruction.




ITEM CODE:CV04F\*

## INTRODUCER SHEATH

- ⊙ Primarily used to introduce balloon, electrode, diagnostic and other catheters into femoral vessels for diagnostic and therapeutic intervention in the coronary arteries.
- ⊙ Kink resistant and flexible sheath. Coated sheath for smooth insertion.
- ⊙ Dilator with curve memory effect for easy sheath placement. Excellent visibility under fluoroscopy.
- ⊙ Sheaths are available in 7cm, 11cm and 25cm lengths with French sizes ranging from 4-9F. All sheaths are sold with dilators.
- ⊙ Dilator lengths are 17cm (11cm sheath) and 31cm (25cm sheath).

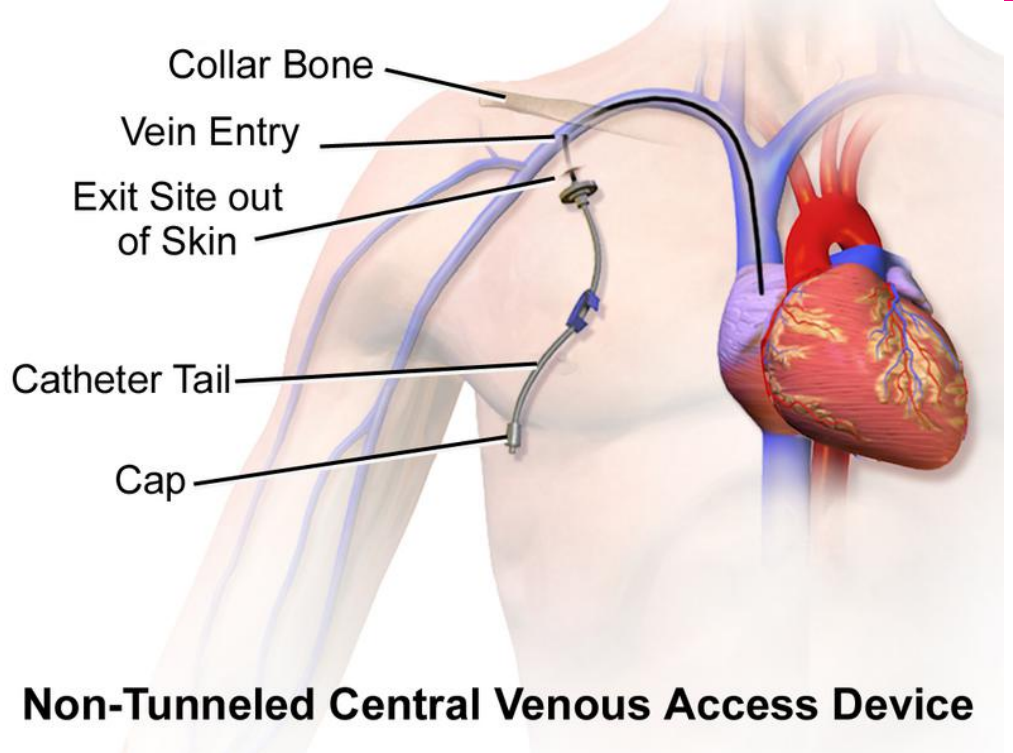

## Lumen Variants of Auracath® Catheters

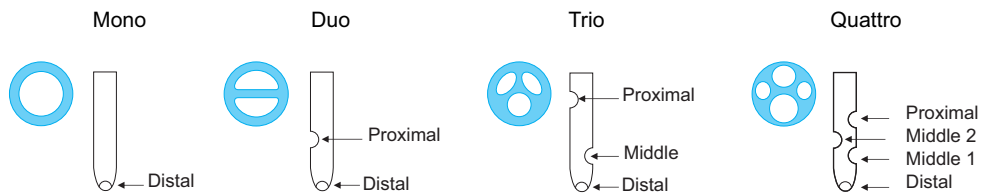

ITEM CODE:CC01F\*

PRESCRIPTION

PATIENT ACCESS

PREPARATION

APPLICATION

DISCHARGE  
MANAGEMENT

# Auracath®


Central Venous Catheter Sets



ITEM CODE:IT10C\*

## PRESSURE MONITORING KIT

- ⦿ Customised Design kit as per user specifications and requirement option of Closed loop blood sampling kit available including needle less sampling site
- ⦿ DEHP Free tubing
- ⦿ Contact for non-obligatory schematic design / samples
- ⦿ Schematic design of
  - AUPMK-S01 (Standard Single Kit)
  - AUPMK-D01 (Standard Double Kit)
  - AUPMK-T01 (Standard Triple Kit)

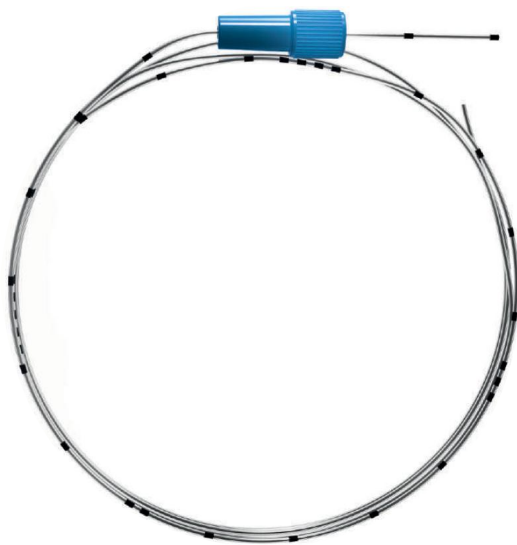

## Epidural Catheter Set


An epidural catheter is a very fine plastic catheter (tube) that is placed through the skin into the epidural space in your spine. This temporary catheter is left in place for a defined period of time; normally less than two weeks.

**An epidural is commonly called the following terms:**


- ⦿ Epidural anesthesia.
- ⦿ Epidural block.
- ⦿ Epidural steroid injection (ESI).
- ⦿ Regional anesthesia.
- ⦿ Neuraxial anesthesia.
- ⦿ The type of anesthetic drug your provider uses.
- ⦿ The concentration of the drug (how strong it is).
- ⦿ The dosage of the drug.

# NEPHROLOGY

NEPHROLOGY

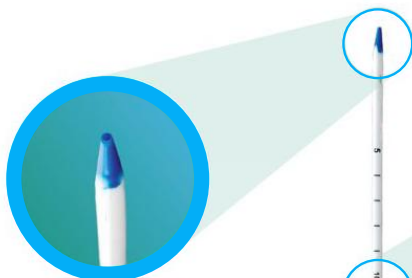

**SOFT TIP**  
allows for easy insertion



**LARGE SIDE HOLES**  
improve blood flow  
and reduce clotting



**ROTATING SUTURE WINGS**  
for secure external anchoring




**CLAMP INSERTS**  
indicate priming volume



## HEMODIALYSIS CATHETER KIT

- ⊙ Indwelling catheter made of specially formulated polyurethane ensures smooth catheter insertion and better bio-compatibility.
- ⊙ Catheter provide desired strength during insertion, softens at body temperature, thus reducing the risk of vascular trauma, kink free nitinol guide Wire prevents the vessel perforation and also provide good torque to ensure firm insertion.
- ⊙ Radio-Opaque catheter tip with clear graduation marking.
- ⊙ Hemodialysis catheter are single/double/multiple lumen catheter that provides temporary vascular access for hemodialysis until a permanent access is available or until another type of dialysis therapy is substituted.
- ⊙ Available in 6.5 FR to 12FR.

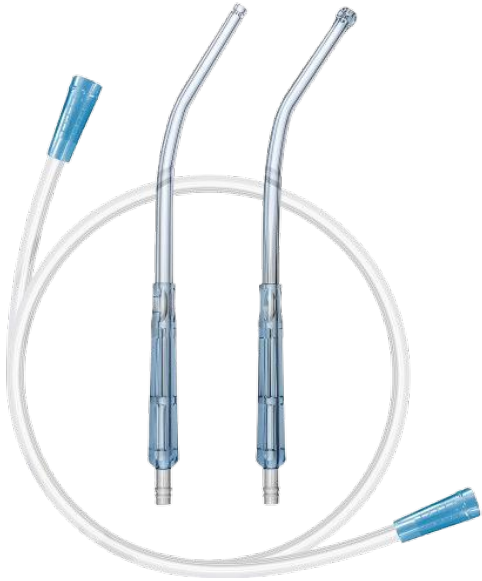

ITEM CODE:SD01B\*

## YANKUR SUCTION SET -STANDARD TIP

- ⊙ Used for the suction from thoracic cavity or/ and operation site during surgery.
- ⊙ 2.5 meter long flexible kink resistant tube with a length for unobstructed drainage provided with or without vacuum thumb control
- ⊙ **Available in set, Tubing only and handle only variants**



ITEM CODE:SD02G\*

## CLOSED WOUND DRAINAGE SET

- ⊙ Drainage from closed wound under negative pressure (sizes 10-18FG) Smooth and traumatic multiple eyes for easy drainage and prevents Post-operative trauma.
- ⊙ Leak proof cap and single step pinch clamp for easy and one hand operation



ITEM CODE:UL02C\*

## LATEX FOLEY CATHETER SILICON COATED 2 WAY & 3 WAY

- ⊙ **Foley Catheter Balloon Catheter–**  
2 Way Foley Catheter (Latex, Silicon Coated)  
Pediatric Size : 6,8 & 10 FG (Two way)
- ⊙ **Adult Size :** 12 to 24 FG (Two way)  
3 Way Foley's Catheter  
(Latex, Silicon Coated)
- ⊙ **Adult Sizes:** 16 to 24 FG (Three way)



ITEM CODE:UL03B\*

## AUR- U METER

- ⊙ Urine collection bag with measuring chamber 250 ML, Specially designed to measure accurate output volume of urine hourly.
- ⊙ This chamber connected to 2000 ml Urine bag.



ITEM CODE:UL01B\*

## URINE BAG

- ⊙ Collection of urine from the patients for diagnostic and/ or treatment available bag capacity of 2000ml urine.
- ⊙ Most suitable for closed urine drainage system for short term use.
- ⊙ Made of medical grade Non-toxic, Bio-compatible P.V.C with top outlet and hanger.



ITEM CODE:GE01C\*

## PVC RYLES TUBE

- ⦿ For aspiration of intestinal fluid or for administration of internal nutrition. 105 cm tube.
- ⦿ Marking at 500mm, 600mm & 700mm from the tip for proper placement.



ITEM CODE:GE02C\*

## INFANT FEEDING TUBE

- ⦿ Used for the nutritional feeding of neonates and paediatric nutritional supplement.
- ⦿ Made up of medical grade Non-toxic, Bio-compatible PVC.
- ⦿ Radio opaque line is provided throughout the length for X-Ray visualization, 50cm.
- ⦿ **Available in Plain and with Graduated scale.**



ITEM CODE:GE06C\*

## STOMACH TUBE

- ⦿ Used for the nutritional feeding. 4 Lateral eyes are provided for efficient aspiration and administration. 125cm tubing.

# ANAESTHESIA & RESPIRATORY CARE



ITEM CODE:AR01A\*

## SILICON MANUAL RESUSCITATORS

- ⊙ Made from 100% silicon, autoclavable, Complete kit has star lumen oxygen tube, reservoir bag, Silicon mask, resuscitator bag and pressure release valve.

Adult	1600ml
Pediatric	500ml
Neonate	250ml



ITEM CODE:AR02B\*

## AURNEB - Nebuliser Mask

Adult/Pediatric/ Neonate with star lumen tubing

- ⊙ Disposable nebulizer mask with chamber & tube for nebulization, Soft, large, anatomical shaped face mask fits comfortably over face.
- ⊙ Nose clip for easy adjustment over patient nose. kink resistant, star lumen, anti-crush tube.
- ⊙ Tube length-200cm.
- ⊙ Available in Adult/Paediatric/ Neonate variants.




ITEM CODE:AR03B\*

## AUXY SET - Oxygen Mask

Adult/Pediatric/ Neonate with star lumen tubing

- ⊙ Oxygen mask with star lumen tube, Elastic strap provided to position the mask properly.
- ⊙ Tube length- 200 cm.
- ⊙ Sizes available are Adult, Paediatric and Infant.

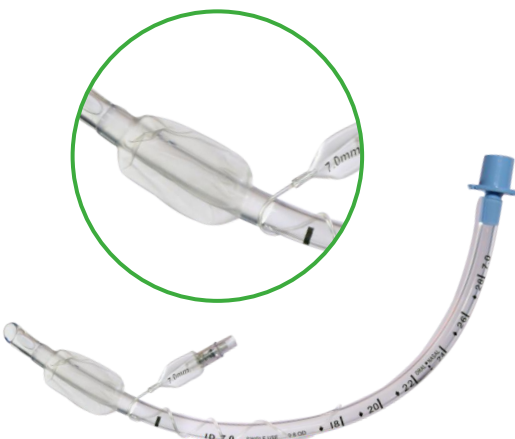


## ENDOTRACHEAL TUBE

- ⊙ Endotracheal tube is used for general anesthesia, intensive care and emergency medicine for airway management and mechanical ventilation, with Naso-Oral tip.
- ⊙ RO line throughout the tube length for X-ray detection of proper placement of the device.
- ⊙ Murphy eye with smooth edges and tip to reduce any trauma to the patient.
- ⊙ High-volume, low-pressure cuff to build an air tight grip between tube and trachea to avoid any leakages. Inflation tube connected with cuff to inflate and deflate it, is kink resistant to ensure patient safety during Procedure.
- ⊙ Available in Plain/Cuffed



# CERTIFICATES



**Certificate of Compliance**  
 Certificate Number: UQ-2022032261

This is to certify that  
**AURUS MEDTECH PRIVATE LIMITED**  
 at  
 Plot No. 140, Sector-68, IMTB, Faridabad-121004, Haryana, India

Has successfully implemented the Quality management System and been found working satisfactorily as per the norms of "Good Manufacturing Practice" as laid down by World Health Organisation "which has been in conformance to the requirements of

**WHO-GMP**

Scope: Central Venous Catheter, Hemodialysis Catheter, Introducer Sheath, Hypodermic & Auto-disable syringes, Sterilized and Single Use Medical Devices- Infusion Set, Blood Transfusion Set, Measured Volume Set, Extension Line, 3-Way Stop Cock, I V Cannula, Foley Catheter & Endotracheal Tube.

This certificate is issued under the following conditions:  
 1. It applies only to the quality system maintained in the manufacture of above referenced Medical Products.  
 2. The certificate remains valid until the manufacturing conditions or the quality systems are changed and is subject to continuous surveillance according to the WHO-GMP Guidelines.  
 3. The certificate validity is conditioned by positive results or surveillance audits.

Validity of this certificate can be verified at [www.ukcertifications.org.uk/verify](http://www.ukcertifications.org.uk/verify)

Date of Certification	22 <sup>nd</sup> March 2022
1 <sup>st</sup> Surveillance Audit Due	21 <sup>st</sup> March 2023
2 <sup>nd</sup> Surveillance Audit Due	21 <sup>st</sup> March 2024
Certificate Expiry (subject to the company maintaining its system to the required standard)	21 <sup>st</sup> March 2025

*Daniel*  
 Authorised Signatory

This certificate is the property of UK Certification & Inspection Limited and shall be returned immediately on request.  
 71-75 Shelton Street, Covent Garden, London, WC2H 9JQ, United Kingdom  
 Website: [www.ukcertifications.org.uk](http://www.ukcertifications.org.uk), email: [info@ukcertifications.org.uk](mailto:info@ukcertifications.org.uk)  
 Company No: 1184782



**Certificate of Compliance**  
**CE**

We hereby declare that the technical file of product complied with the requirement of Medical Device Regulation "Council Regulation 2017/745".  
 Certificate No. CE-5863

Manufacturer  
 Name : AURUS MEDTECH PRIVATE LIMITED  
 Address : Plot No. 140, Sector -68, IMT, Faridabad, HSIDC, Haryana-121004, India

Products : PRODUCTS DETAILS AS PER APPENDIX-1

Complies with the requirements applicable to it  
 The quality system (as has been assessed, approved and is subject to continuous surveillance according to the Medical Device Regulation "Council Regulation 2017/745)

This certificate is issued under the following conditions:  
 1. It applies only to the quality system maintained in the manufacture of above referenced models and it does not substitute the design or type-examination procedures, if requested.  
 2. The certificate remains valid until the manufacturing conditions or the quality systems are changed.  
 3. The certificate validity is conditioned by positive results or surveillance audits.  
 The CE mark as shown above can be used, under the responsibility of the manufacturer, after completion of an EC Declaration of conformity and compliance with all relevant EC Directives. The statement is based on a single evaluation of one sample of above mentioned product. It does not imply an assessment of the whole production.

Validity of this certificate can be verified at [www.ukcertifications.org.uk/verify](http://www.ukcertifications.org.uk/verify)

Date of Certification	22 <sup>nd</sup> July 2024
1 <sup>st</sup> Surveillance Audit Due	21 <sup>st</sup> July 2025
2 <sup>nd</sup> Surveillance Audit Due	21 <sup>st</sup> July 2026
Certificate Expiry (subject to the company maintaining its system to the required standard)	21 <sup>st</sup> July 2027

*Daniel*  
 Authorised Signatory

This certificate is the property of UK Certification & Inspection Limited and shall be returned immediately on request.  
 71-75 Shelton Street, Covent Garden, London, WC2H 9JQ, United Kingdom  
 Website: [www.ukcertifications.org.uk](http://www.ukcertifications.org.uk), email: [info@ukcertifications.org.uk](mailto:info@ukcertifications.org.uk)  
 Company No: 1184782



**CERTIFICATE OF REGISTRATION**

This is to certify that the management system of  
**Aurus MedTech Private Limited**

Main site: Plot-140, Sector-68, IMT, Faridabad, HSIDC, Faridabad, Haryana, 121004, India

has been registered by Intertek as conforming to the requirements of


**EN ISO 13485:2016**  
**ISO 13485:2016**

The management system is applicable to:  
 Design, development and manufacture of sterile/non-sterile Nonactive Medical Disposable Devices for the area of infusion therapy, perfusion therapy and general surgery.

Certificate Number: 0247551  
 Revision: 00  
 Initial Certification Date: 20 April 2023  
 Date of Certification Decision: 20 April 2023  
 Certificate Valid Date: 20 April 2023  
 Certificate Expiry Date: 19 April 2026

Intertek  
 Brian Mather  
 Certification Authority, Intertek Medical Notified Body #1  
 Intertek Medical Notified Body #1  
 P.O. Box 1101, St. 154 22 Kuala, Sweden

CERTIFICATE NO:  
**DIPP85413**

  
 Government of India  
 Ministry of Commerce & Industry  
 Department for Promotion of Industry and Internal Trade

**#startupindia**

**CERTIFICATE OF RECOGNITION**

This is to certify that **AURUS MEDTECH PRIVATE LIMITED** incorporated as a **Private Limited Company** on **11-01-2021**, is recognized as a startup by the Department for Promotion of Industry and Internal Trade. The startup is working in 'Healthcare & Lifesciences' Industry and 'Medical Devices Biomedical' sector as self-certified by them.

This certificate shall only be valid for the Entity up to **Ten years** from the date of its incorporation only if its turnover for any of the financial years has not extended ₹ 100 Cr.

25-08-2021      10-01-2031  
 DATE OF ISSUE      VALID UPTO



# AurusMedTech Pvt. Ltd.

**Corporate Office :** 704 & 704A Narain Manzil,  
Barakhamba Road, Delhi-110001

**Plant :** Plot No-140, IMT Sector-68 HSIIDC,  
Faridabad, Haryana-121004, India



✉ [sales@aurusmedtech.com](mailto:sales@aurusmedtech.com) 🌐 [www.aurusmedtech.com](http://www.aurusmedtech.com) ☎ +91 129 4000439

